

# INTRODUCTION TO CO<sub>2</sub> MEASUREMENTS IN SEA WATER

ANDREW G. DICKSON  
SCRIPPS INSTITUTION OF OCEANOGRAPHY, UC SAN DIEGO



# METHODS FOR MEASURING THE CO<sub>2</sub> PARAMETERS IN SEA WATER

---

---

# USUAL PARAMETERS MEASURED

---

- Total dissolved inorganic carbon

$$C_T = [\text{CO}_2] + [\text{HCO}_3^-] + [\text{CO}_3^{2-}]$$

- Total hydrogen ion concentration (pH)

$$\text{pH} = -\lg [\text{H}^+]$$

- Partial pressure of  $\text{CO}_2$  (in air in equilibrium with sea water)

$$p(\text{CO}_2) = x(\text{CO}_2) p = [\text{CO}_2] / K_0$$

- Total alkalinity

$$A_T = [\text{HCO}_3^-] + 2[\text{CO}_3^{2-}] + [\text{B}(\text{OH})_4^-] + [\text{OH}^-] - [\text{H}^+]$$

	Advantages	Disadvantages
$C_T$	<p><i>T, p independent</i></p> <p>Unambiguous interpretation of changes</p>	<p>Needs care with sample handling</p> <p><i>No autonomous system available</i></p>
pH	<p><i>Autonomous systems available</i></p> <p>Master variable?</p>	<p><i>Function of T, p</i></p> <p>Needs care with sample handling</p> <p>Interpretation problems</p>
$p(\text{CO}_2)$	<p><i>Autonomous systems available</i></p>	<p><i>Function of T, p</i></p> <p>Changes not easy to interpret</p>
$A_T$	<p><i>T, p independent</i></p> <p>Often possible to interpret changes</p>	<p><i>No autonomous system available</i></p> <p>Harder to interpret in some systems</p>

# TOTAL DISSOLVED INORGANIC CARBON

---

- Carbon dioxide mass balance equation

$$C_T = [\text{CO}_2] + [\text{HCO}_3^-] + [\text{CO}_3^{2-}] \quad T, p \text{ independent}$$

UNITS: moles per kilogram of solution (usually  $\mu\text{mol kg}^{-1}$ )

# TOTAL DISSOLVED INORGANIC CARBON

---

- Carbon dioxide mass balance equation



1. Acidify a known amount of sample
2. Extract the  $\text{CO}_2$
3. Measure the amount of  $\text{CO}_2$ 
  - Coulometry
  - Infra-red analyzer
  - Other

# COMPARISON OF TECHNIQUES

---

---

	Advantages	Disadvantages
<i>IR system</i>	<p>Cheaper system Faster sample throughput Less waste disposal Less <i>start-up</i> time Smaller sample ?</p>	<p>Lower reproducibility Calibration not v. stable Limited collaborative testing as yet</p>
<i>Coulometry system</i>	<p>Higher reproducibility Stable calibration Well tested in many labs</p>	<p>Slower sample throughput Proprietary coulometer solution (hazardous) Significant <i>start-up</i> time needed</p>

# TOTAL HYDROGEN ION CONCENTRATION (pH)

---

- Species concentration,  $[H^+]$

$$pH = -\lg [H^+]$$

*T, p dependent*

UNITS: pH is dimensionless

But, total hydrogen ion concentration is in moles per kilogram of solution



# TOTAL HYDROGEN ION CONCENTRATION (pH)

---

- Species concentration,  $[H^+]$

$$pH = -\lg [H^+]$$

*T, p dependent*

1. Electrometric measurement of pH
2. Spectrophotometric measurement of pH

# ELECTROMETRIC pH MEASUREMENT

---

A direct electrometric technique using an electrode sensitive to hydrogen ion in a “pH cell”;

The Nernst equation underlies this approach to measuring pH:

$$E = E^*(S, T, p) - \left( \frac{RT \ln 10}{F} \right) \lg[H^+]$$

$$= E^*(S, T, p) + \left( \frac{RT \ln 10}{F} \right) \text{pH}$$

$$\text{pH}(X) = \text{pH}(S) - \frac{E_x - E_s}{RT \ln 10 / F}$$

For this operational approach to give an accurate estimate of  $[H^+]$ , it is essential that the calibration standard be matched closely to the sample in composition.

**IT RARELY IS !**


To use autonomously (not constant  $S, T, p$ ), it is essential that the functional form of  $E^*(S, T, p)$  be known well.

**IT OFTEN ISN'T!**




# SPECTROPHOTOMETRIC pH MEASUREMENT

A colorimetric technique in which an **indicator dye** is added to the solution and the pH inferred from the resulting absorbance spectrum

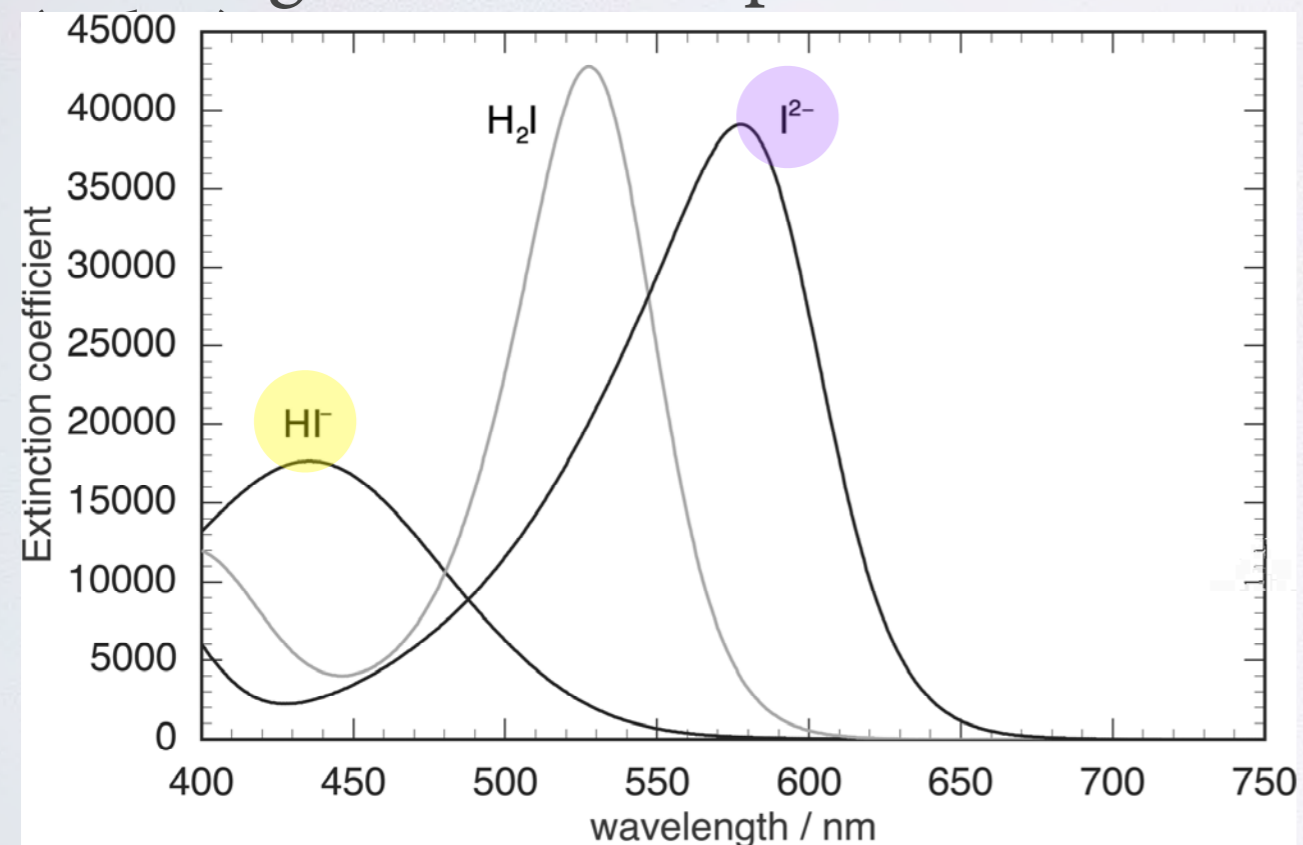

$$\text{pH} = -\lg K(\text{HI}^-) \left( \frac{\epsilon_1(\text{I}^{2-})}{\epsilon_2(\text{HI}^-)} \right) + \lg \left( \frac{A_1 / A_2 - \epsilon_1(\text{HI}^-) / \epsilon_2(\text{HI}^-)}{1 - (A_1 / A) \epsilon_2(\text{I}^{2-}) / \epsilon_1(\text{I}^{2-})} \right)$$

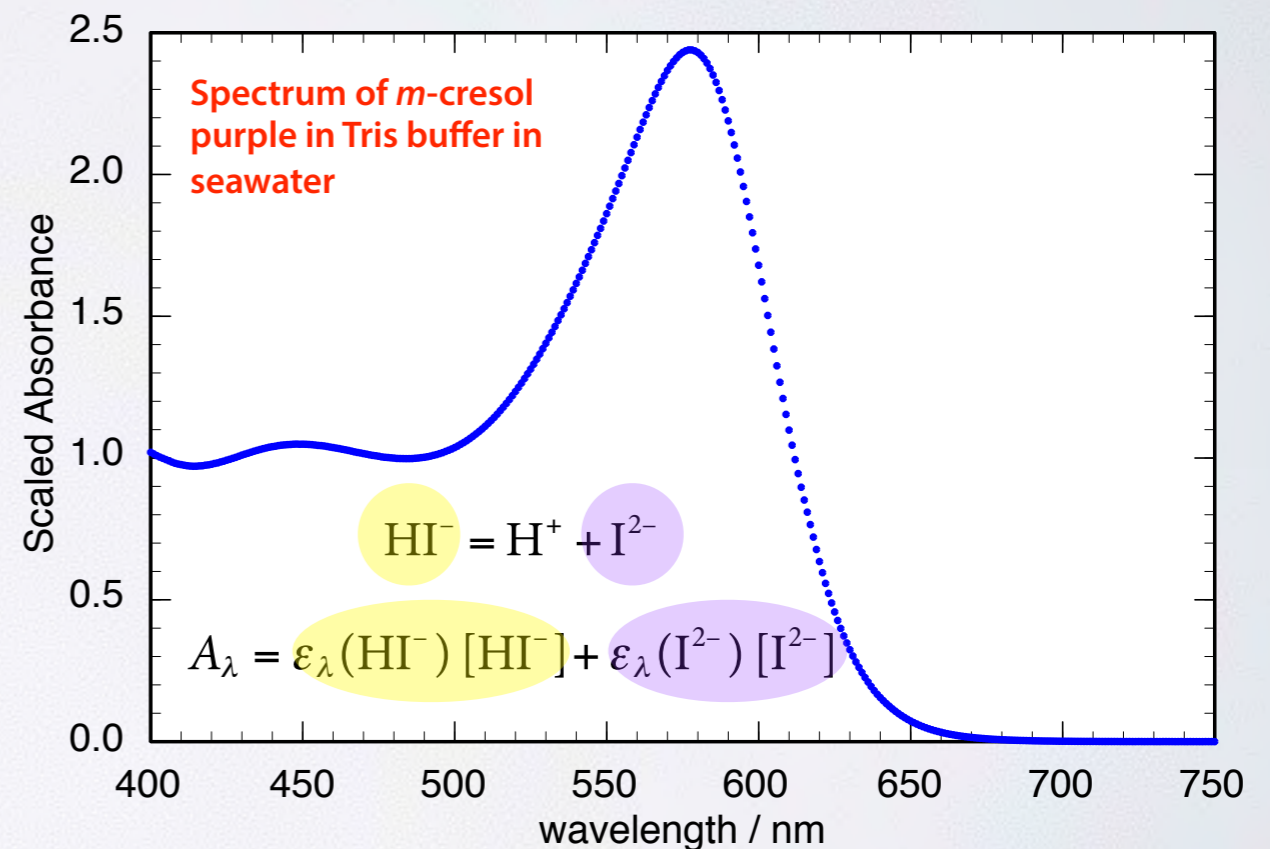


# POTENTIAL IMPLICATIONS OF IMPURE DYE


## Purification and Characterization of meta-Cresol Purple for Spectrophotometric Seawater pH Measurements

I. Byrne\*

140 Seventh Avenue South, St. Petersburg, Florida 33701, United States

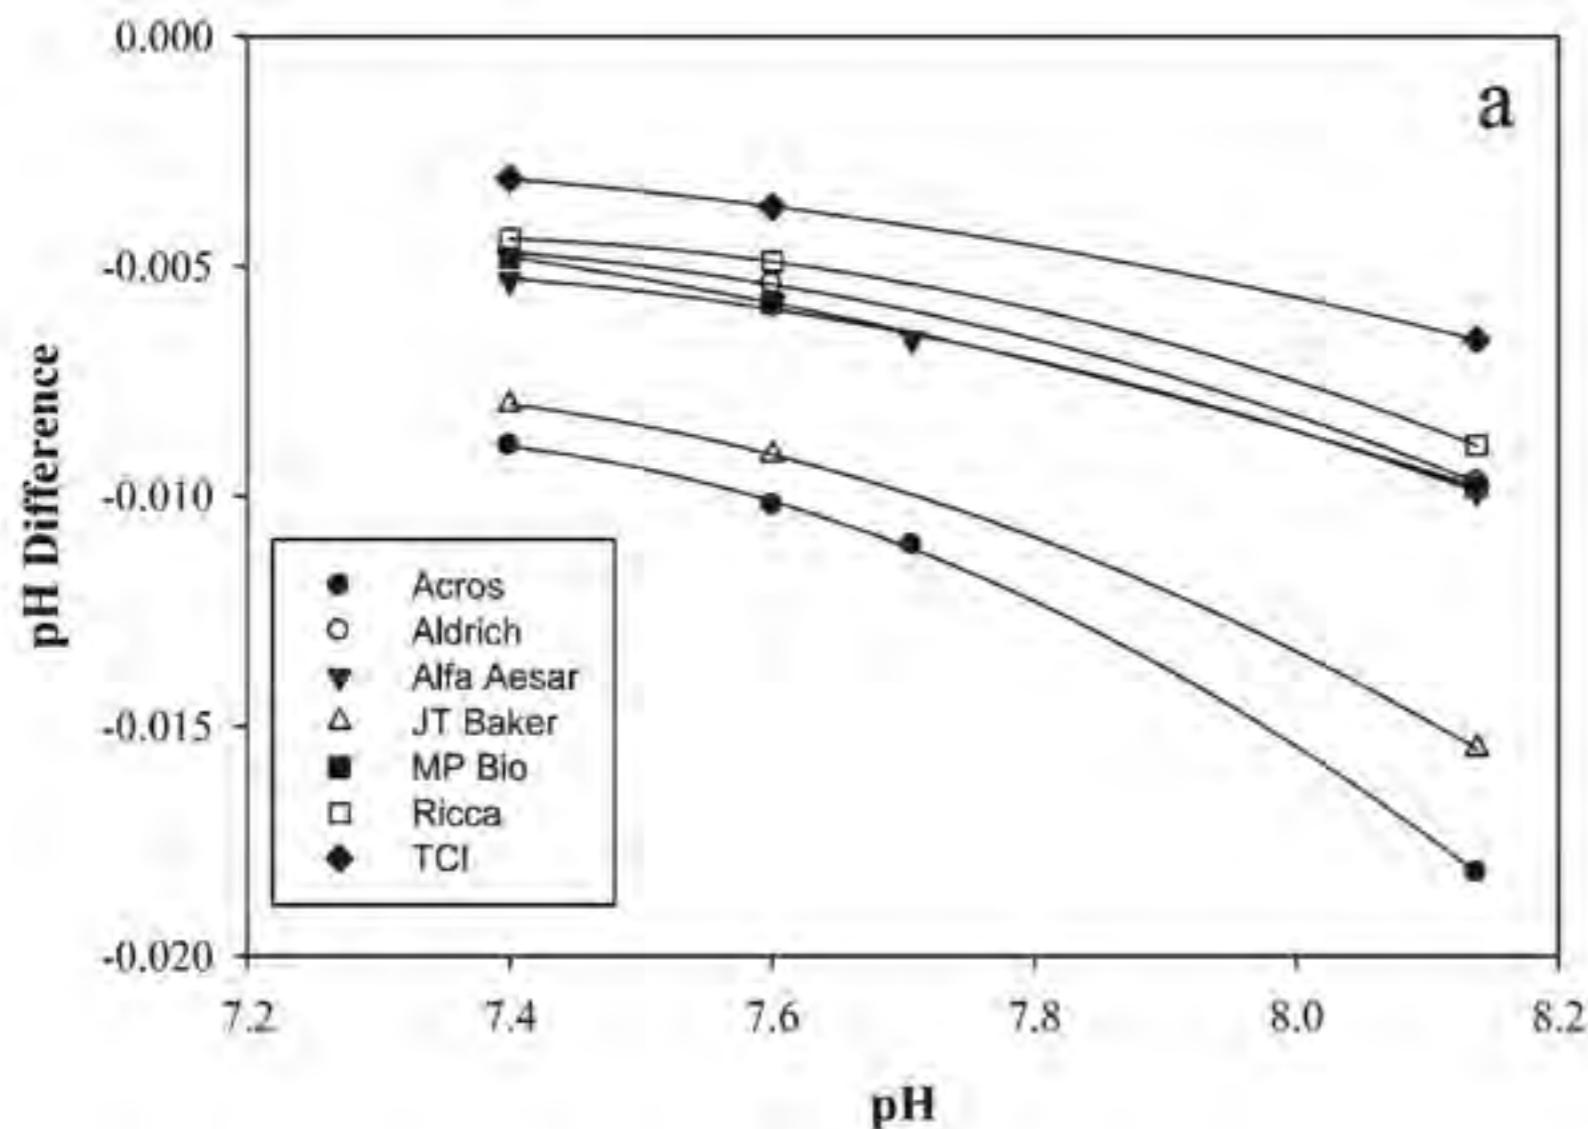

apid and precise measurements of acid–base indicators used in accuracy. This work describes meta-cresol purple (mCP), and thermodynamic equilibrium temperature ( $T$ ) and salinity ( $S$ ). on concentration scale ( $\text{pH}_T$ ) mance ratios ( $R = \lambda_2 A / \lambda_1 A$ ) as

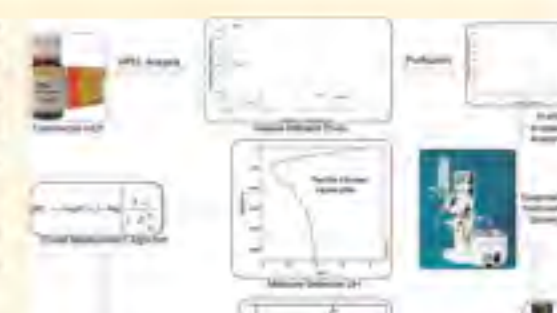

Thus far the uncertainty introduced by dye impurities has only been characterized at a single temperature (25 °C) and salinity (35).

# COMPARISON OF TECHNIQUES

---

	Equipment Cost	Ease of use	Uncertainty in best labs
Electrometric pH cell	Relatively cheap (need $T$ control)	Simple to use, needs regular recalibration*	0.02 limited availability of RMs
Using indicator & spectrophotometer	Mid-range k\$ 10–25	Can be automated	< 0.01 limited availability of pure mCP


\* The Honeywell DuraFET<sup>®</sup> seems to have a significantly more stable calibration than a conventional pH cell.

# PARTIAL PRESSURE OF CO<sub>2</sub>

(IN AIR THAT IS IN EQUILIBRIUM WITH THE WATER SAMPLE)

---

- Species concentration, [CO<sub>2</sub>]



$$K_0(T, p, S) = \frac{[\text{CO}_2]}{x(\text{CO}_2) \cdot p}$$

mole fraction of CO<sub>2</sub>

equilibration pressure

$$p(\text{CO}_2) = x(\text{CO}_2) p = [\text{CO}_2] / K_0$$

*T, p dependent*

UNITS: pressure units (usually  $\mu\text{atm}$ )

# PARTIAL PRESSURE OF CO<sub>2</sub>

(IN AIR THAT IS IN EQUILIBRIUM WITH THE WATER SAMPLE)

---

- Species concentration, [CO<sub>2</sub>]

$$p(\text{CO}_2) = x(\text{CO}_2) p = [\text{CO}_2] / K_0$$

*T, p dependent*

## A. Gas phase equilibration

- Measure  $x(\text{CO}_2)$  in the gas phase using NDIR
- Measure  $x(\text{CO}_2)$  in the gas phase using GC

## B. Membrane equilibration (with gas or external solution)

- Measure  $x(\text{CO}_2)$  in the gas phase using NDIR
- Measure pH in external solution (*see pH section*)

# COMPARISON OF TECHNIQUES

---

	Equipment Cost	Advantages / Disadvantages	Uncertainty*
infra-red analyzer	\$30,000 – \$60,000	Quality depends mostly on design of equilibrators	With careful calibration < 0.5%
pH-based analyzer	~\$25,000	Awkward to calibrate Membrane can foul	Can be 1–2%

\* These values are for commercial systems when working well.



# TOTAL ALKALINITY

---

$$A_T = [\text{HCO}_3^-] + 2[\text{CO}_3^{2-}] + [\text{B(OH)}_4^-] + [\text{OH}^-] - [\text{H}^+]$$

*T, p independent*

UNITS: moles per kilogram of solution (usually  $\mu\text{mol kg}^{-1}$ )

# TOTAL ALKALINITY

---

- Hydrogen ion mass-balance equation

$$A_T = [\text{HCO}_3^-] + 2[\text{CO}_3^{2-}] + [\text{B(OH)}_4^-] + [\text{OH}^-] - [\text{H}^+] \quad T, p \text{ independent}$$

## Acidimetric titration

- Closed-cell
  - Open-cell
- a. Can also add acid in one aliquot (single point method)
  - b. Can use either a pH cell or spectrophotometry to estimate  $[\text{H}^+]$  during titration.
  - c. Ideally use NLLS to locate equivalence point; can use Gran technique

# COMPARISON OF TECHNIQUES

---

	Equipment Cost	Advantages / Disadvantages	Uncertainty*
Closed cell	~\$30,000	Uses cell to measure $V$ Problems with back-pressure	~2-4 $\mu\text{mol kg}^{-1}$
Open cell	\$15,000 to \$30,000	Can be very precise Easier to diagnose faults	~1-4 $\mu\text{mol kg}^{-1}$

\* These values are for commercial systems when working well.

# STATUS OF CURRENT MEASUREMENT PRACTICE

---

---

# SAMPLING & ANALYSIS STRATEGIES

---

Discrete samples (collected from desired locations, preserved, then analyzed later in a laboratory)

Automated on-line analysis (*e.g.* a stream of sea water pumped into the instrument)

Instruments operated in a profiling mode, *e.g.* as part of a CTD package

Autonomous instruments able to carry out their analyses remotely in the ocean

# DEVELOPMENT STATE OF CO<sub>2</sub> MEASUREMENT SYSTEMS

---

Level 0 – No working system available

Level 1 – Prototype system available in single lab

Level 2 – 2nd generation prototype in use

Level 3 – Home-built systems in a number of labs

Level 4 – Can be purchased commercially

Level 5 – Commercially available, reliable, and fully supported

# DEVELOPMENT STATE OF CO<sub>2</sub> MEASUREMENT SYSTEMS

	Discrete samples	Autonomous sampling & analysis	Profiling instrument	Remote instruments in ocean
$C_T$	3/4/5?	1/2	0	0/1
pH	3/4	3/4/5?	1/2	3/4/5?
$p(\text{CO}_2)$	2	3/4/5	1	3/4/5
$A_T$	3/4/5?	1/4	0	0/1

# ESTIMATED UNCERTAINTIES<sup>†</sup> FOR DISCRETE MEASUREMENTS

	State-of-the-art laboratory	State-of-the-art at-sea lab (suitable RMs)	Other laboratories (suitable RMs)	Laboratories not using RMs
$C_T$	1.0 $\mu\text{mol kg}^{-1}$	2 $\mu\text{mol kg}^{-1}$	4–10 $\mu\text{mol kg}^{-1}$	?
pH	0.010 (0.003 ?)	0.010 (0.003 ?)	0.01–0.05	?
$p(\text{CO}_2)$ IR-based	1.0 $\mu\text{atm}$	2 $\mu\text{atm}$	5–10 $\mu\text{atm}$	?
$A_T$	1.2 $\mu\text{mol kg}^{-1}$	2 $\mu\text{mol kg}^{-1}$	4–10 $\mu\text{mol kg}^{-1}$	?

<sup>†</sup> Based on measuring surface oceanic  $\text{CO}_2$  levels






Contents lists available at ScienceDirect

## Marine Chemistry

journal homepage: [www.elsevier.com/locate/marchem](http://www.elsevier.com/locate/marchem)

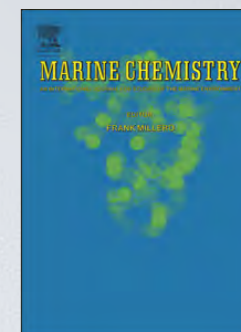

# An inter-laboratory comparison assessing the quality of seawater carbon dioxide measurements

Emily E. Bockmon <sup>\*</sup>, Andrew G. Dickson

Marine Physical Laboratory, Scripps Institution of Oceanography, University of California, San Diego, 9500 Gilman Drive, La Jolla, CA 92093-0244, USA



Will make available in the **Dropbox**

### ARTICLE INFO

#### Article history:

Received 25 April 2014

Received in revised form 7 January 2015

Accepted 4 February 2015

Available online 11 February 2015

#### Keywords:

Carbonate chemistry

Intercomparison

Carbon dioxide

Alkalinity

Dissolved inorganic carbon

pH

Ocean acidification

### ABSTRACT

Seawater CO<sub>2</sub> measurements are being made with increasing frequency as interest grows in the ocean's response to changing atmospheric CO<sub>2</sub> levels and to climate change. The ultimate usefulness of these measurements depends on the data quality and consistency. An inter-laboratory comparison was undertaken to help evaluate and understand the current reliability of seawater CO<sub>2</sub> measurements. Two seawater test samples of different CO<sub>2</sub> content were prepared according to the usual method for the creation of seawater reference materials in the Dickson Laboratory at Scripps Institution of Oceanography. These two test samples were distributed in duplicate to more than 60 laboratories around the world. The laboratories returned their measurement results for one or more of the following parameters: total alkalinity ( $A_T$ ), total dissolved inorganic carbon ( $C_T$ ), and pH, together with information about the methods used and the expected uncertainty of the measurements. The majority of laboratories reported  $A_T$  and  $C_T$  values for all their measurements that were within 10  $\mu\text{mol kg}^{-1}$  of the assigned values (i.e. within  $\pm 0.5\%$ ), however few achieved results within 2  $\mu\text{mol kg}^{-1}$  (i.e. within  $\pm 0.1\%$ ), especially for  $C_T$ . Results for the analysis of pH were quite scattered, with little suggestion of a consensus value. The high-CO<sub>2</sub> test sample produced results for both  $C_T$  and pH that suggested in many cases that CO<sub>2</sub> was lost during analysis of these parameters. This study thus documents the current quality of seawater CO<sub>2</sub> measurements in the various participating laboratories, and helps provide a better understanding of the likely magnitude of uncertainties in these measurements within the marine science community at the present time. Further improvements will necessarily hinge on adoption of an improved level of training in both measurement technique and of suitable quality control procedures for these measurements.

© 2015 The Authors. Published by Elsevier B.V. This is an open access article under the CC BY-NC-ND license

(<http://creativecommons.org/licenses/by-nc-nd/4.0/>)

# RECENT INTER-LABORATORY PROFICIENCY STUDY

---


Assigned values for total alkalinity, total dissolved inorganic carbon, and pH (25 °C; total scale) for the two test samples. Values are expressed as *mean ± standard deviation (number of analyses)*.

	Batch A	Batch B
Salinity	33.190	33.186
Total alkalinity	2215.08 ± 0.49 (24) μmol kg <sup>-1</sup>	2216.26 ± 0.52 (18) μmol kg <sup>-1</sup>
Total dissolved inorganic carbon	2015.72 ± 0.74 (9) μmol kg <sup>-1</sup>	2141.94 ± 0.37 (6) μmol kg <sup>-1</sup>
pH (25 °C; total scale)	7.8796 ± 0.0019 (18)	7.5541 ± 0.0020 (18)


**Normal RM**

**High-CO<sub>2</sub> RM**

# RECENT INTER-LABORATORY PROFICIENCY STUDY

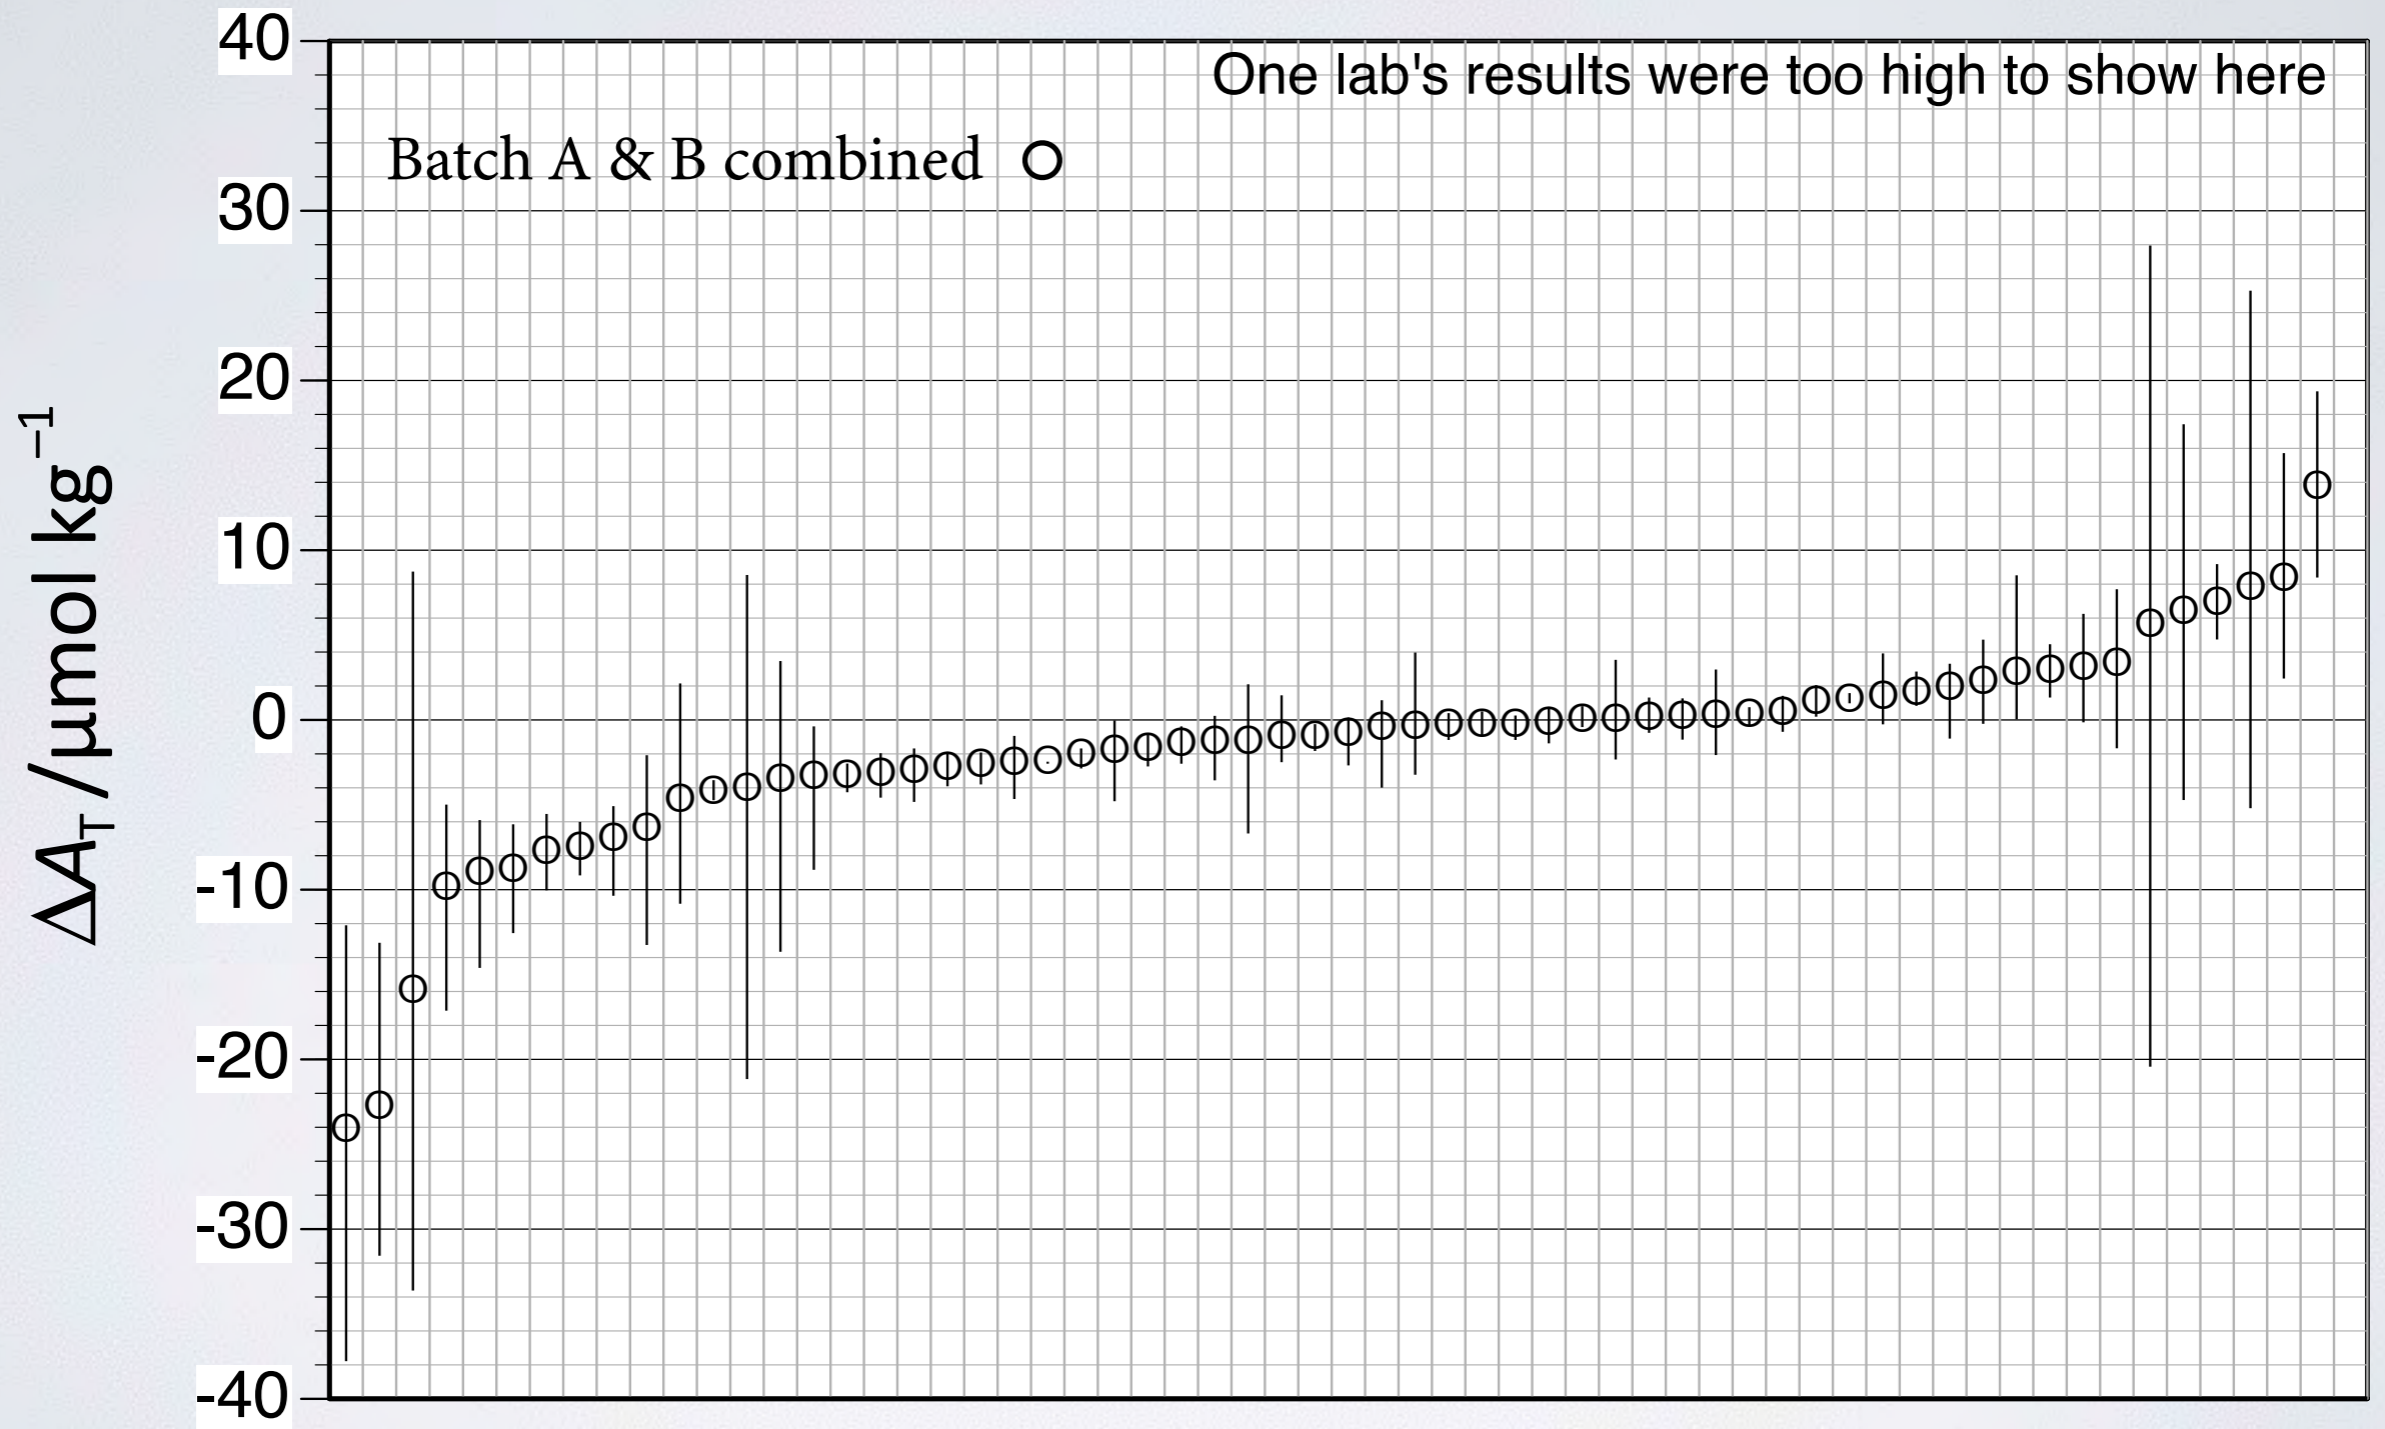


# RECENT INTER-LABORATORY PROFICIENCY STUDY

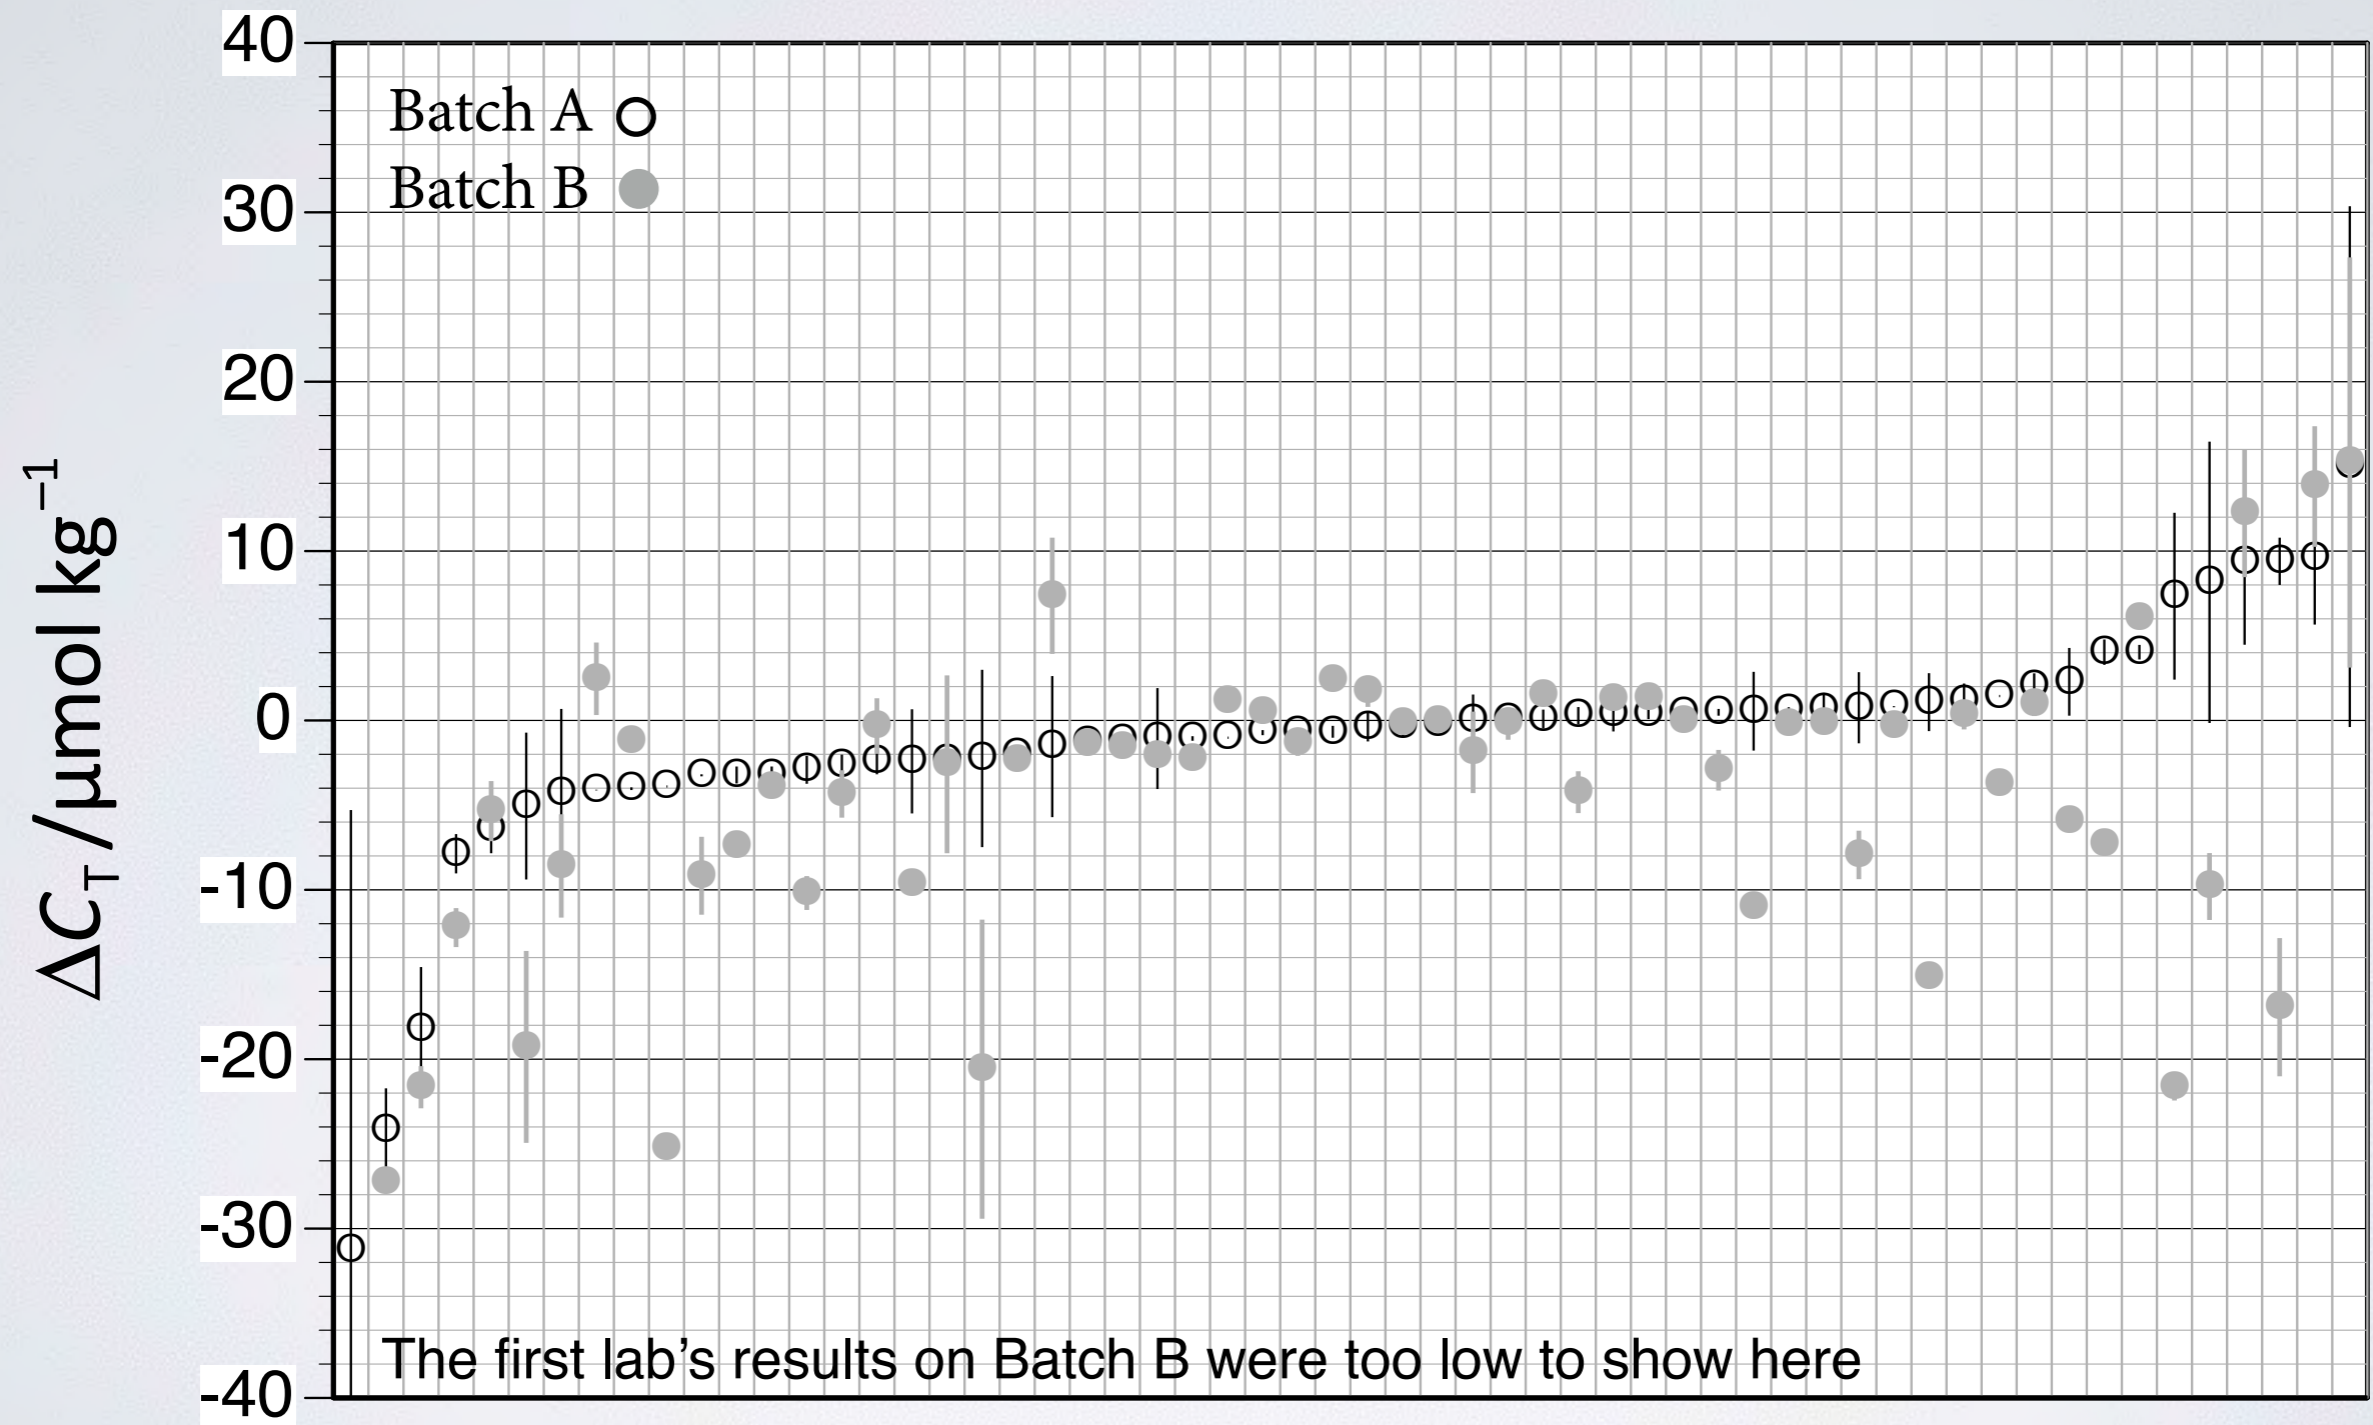


# RECENT INTER-LABORATORY PROFICIENCY STUDY

spectrophotometric

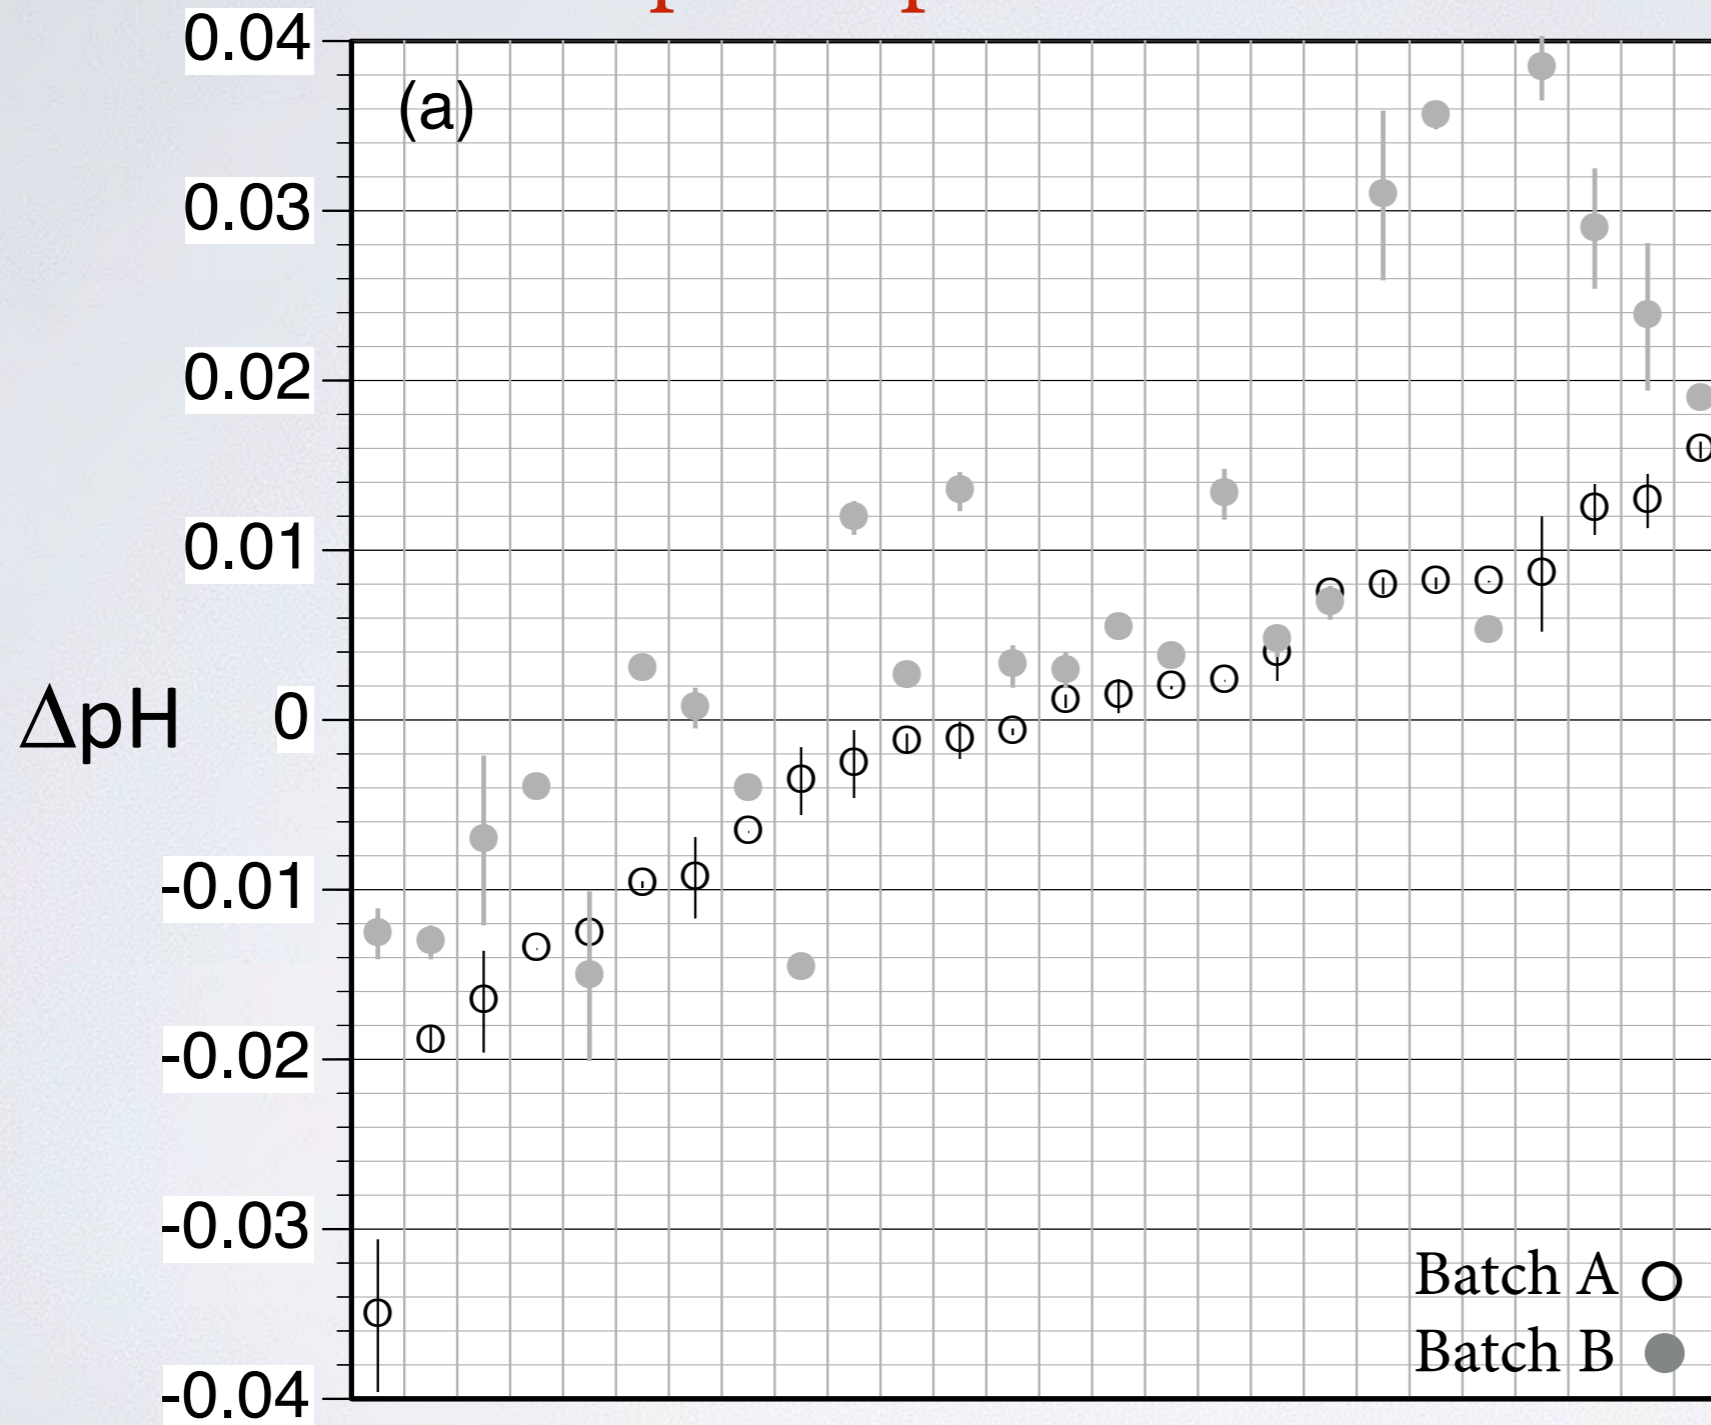

glass electrodes

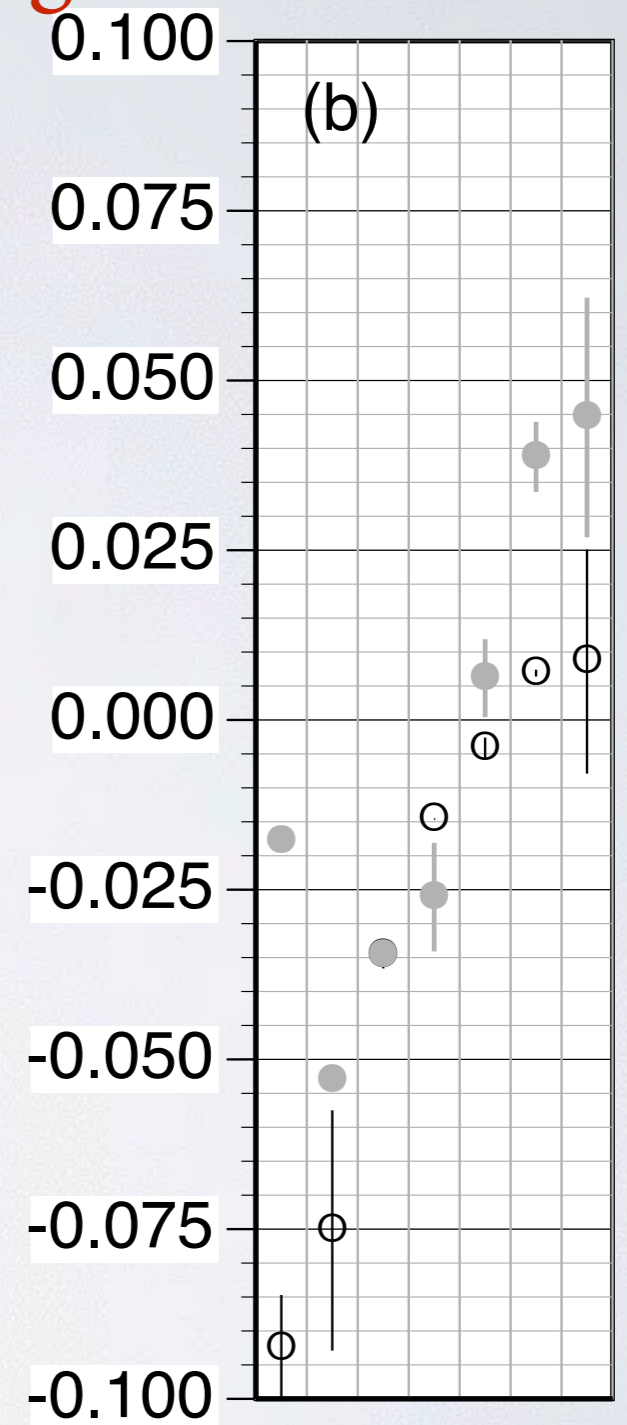

**THINK!**



**THERE MIGHT BE  
A *BETTER* WAY**

# FASTER, BETTER, CHEAPER

---

In 1992, NASA Administrator Daniel Goldin began the agency's "Faster, Better, Cheaper" initiative.


The popular consensus on "Faster, Better, Cheaper" is often expressed in the supposedly self-evident saying: "faster, better, cheaper — pick two."

Is this necessarily true for seawater carbonate system measurements?

We clearly understand the meanings of "faster" and "cheaper", but how should we define "better"?

# DESIRE FOR HIGH-QUALITY MEASUREMENTS

---

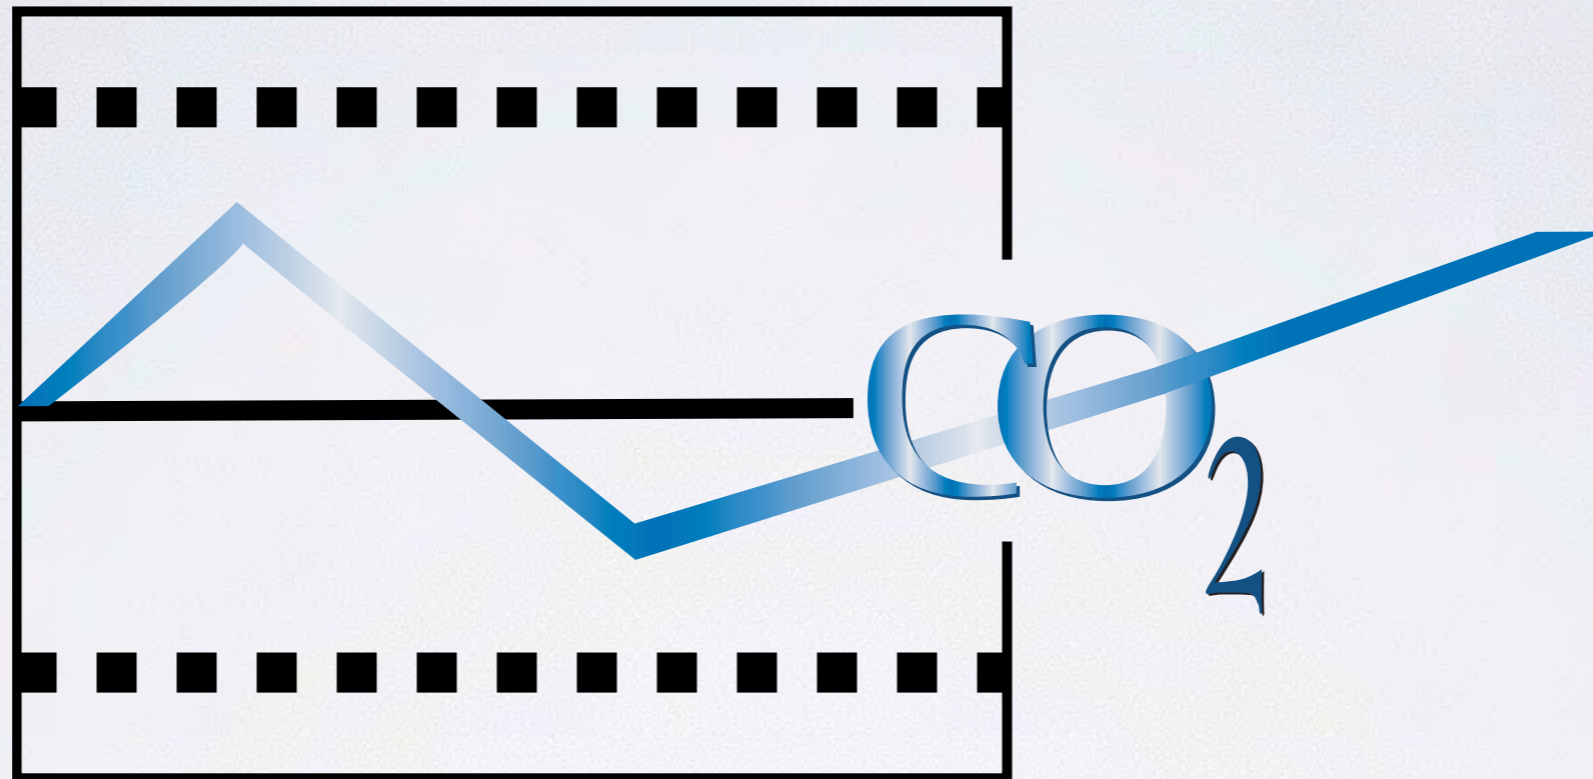



# WHAT IS QUALITY?

---

Quality is fitness for purpose.

*Fitness for purpose*: the property of data produced by a measurement process that enables a user of the data to make technically correct decisions for a stated purpose.

Fitness for purpose therefore refers to the magnitude of the uncertainty associated with a measurement in relation to the needs of the application area.

**Has implications for the level of resources needed!**

# WHEN ASSESSING “BETTER”, UNCERTAINTY IS NOT THE ONLY MEASURE!

---

YOU SHOULD CONSIDER:

1. Overall uncertainty required
2. Cost of measurement(s)
  - a. Cost of equipment (purchase / maintenance)
  - b. Cost of training
  - c. Cost of analysis (time & materials)
3. Convenience of measurement
  - a. Availability of equipment (purchase / maintenance)
  - b. Sample size required
  - c. Time until results are available
4. Cost of making a wrong measurement.

**These procedures are aimed at scientists  
making open ocean measurements**

## Best Practices for CO<sub>2</sub> Measurements

SPECIAL PUBLICATION 3  
SCOR REPORT No. 8



[http://cdiac.ornl.gov/oceans/Handbook\\_2007.html](http://cdiac.ornl.gov/oceans/Handbook_2007.html)

# FOR OPEN-OCEAN MEASUREMENTS

---

YOU SHOULD CONSIDER:

1. Overall uncertainty required AS GOOD AS POSSIBLE!
2. Cost of measurement(s) MONEY NO OBJECT?
  - a. Cost of equipment (purchase / maintenance)
  - b. Cost of training
  - c. Cost of analysis (time & materials)
3. Convenience of measurement WOULD BE NICE!
  - a. Availability of equipment (purchase / maintenance)
  - b. Sample size required
  - c. Time until results are available
4. Cost of making a wrong measurement. VERY HIGH!

# FOR OCEAN ACIDIFICATION MEASUREMENTS

---

YOU SHOULD CONSIDER:

1. Overall uncertainty required STILL NEEDS THOUGHT
2. Cost of measurement(s) BE NICE IT IT WERE CHEAP!
  - a. Cost of equipment (purchase / maintenance)
  - b. Cost of training
  - c. Cost of analysis (time & materials)
3. Convenience of measurement PLEASE!!
  - a. Availability of equipment (purchase / maintenance)
  - b. Sample size required
  - c. Time until results are available
4. Cost of making a wrong measurement. NEEDS THOUGHT

# KEY QUESTIONS TO ASK ABOUT ANY ANALYTICAL METHOD

---

---

# KEY QUESTIONS

---

1. How does the method work?
2. How is it calibrated?
3. What is the overall uncertainty of the measured value?
4. Does it provide the quality I need?
5. What does the method cost to use?

WE SHALL DISCUSS THIS MORE DURING THE WEEK

---

---



